



Picture 1. Cooling of the sensor of digital thermometer with the piece of ice before its contact with the skin surface.

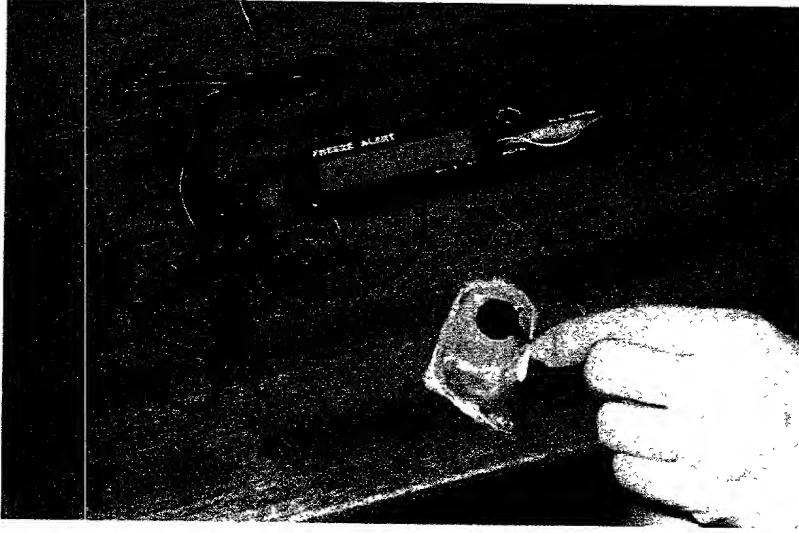


Picture 2. Application of cooled digital thermometer as cold stimuli and measuring device at the same time.

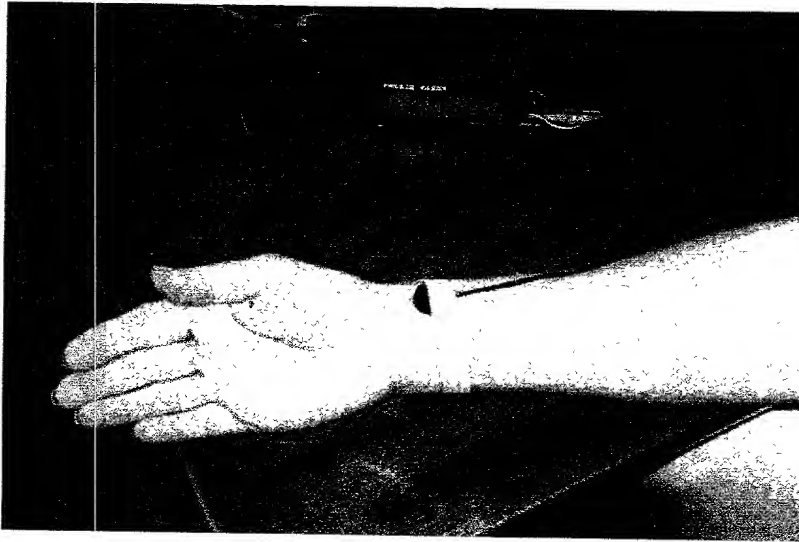


*[Handwritten signature]*



K.K.T.C.  
LEFKOŞA NOTERİ  
05 Kasım 2001  
Enver Sedat Simavi

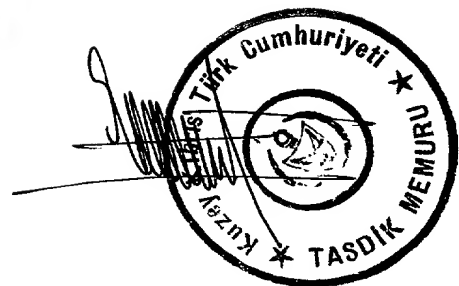

United States Patent & Trademark Office  
Office of Initial Patent Examination -- Scanning Division

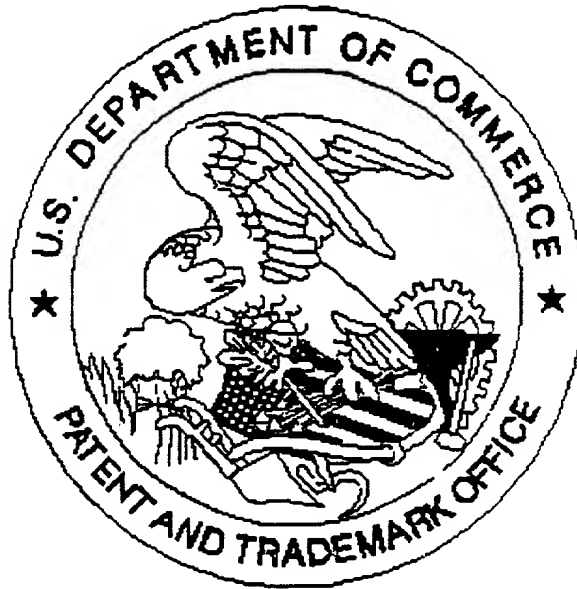

Application deficiencies found during scanning:

☐ Page(s) \_\_\_\_\_ of \_\_\_\_\_ were not present  
for scanning. (Document title)

☐ Page(s) \_\_\_\_\_ of \_\_\_\_\_ were not present  
for scanning. (Document title)

☒ Scanned copy is best available. *photographs are very dark.*